

**Zeitschrift:** Acta Tropica  
**Herausgeber:** Schweizerisches Tropeninstitut (Basel)  
**Band:** 32 (1975)  
**Heft:** 4

**Artikel:** Advantages of X-ray microanalysis in the field of medical mycology  
**Autor:** Thibaut, M. / Ansel, M.  
**DOI:** <https://doi.org/10.5169/seals-312104>

### **Nutzungsbedingungen**

Die ETH-Bibliothek ist die Anbieterin der digitalisierten Zeitschriften auf E-Periodica. Sie besitzt keine Urheberrechte an den Zeitschriften und ist nicht verantwortlich für deren Inhalte. Die Rechte liegen in der Regel bei den Herausgebern beziehungsweise den externen Rechteinhabern. Das Veröffentlichen von Bildern in Print- und Online-Publikationen sowie auf Social Media-Kanälen oder Webseiten ist nur mit vorheriger Genehmigung der Rechteinhaber erlaubt. [Mehr erfahren](#)

### **Conditions d'utilisation**

L'ETH Library est le fournisseur des revues numérisées. Elle ne détient aucun droit d'auteur sur les revues et n'est pas responsable de leur contenu. En règle générale, les droits sont détenus par les éditeurs ou les détenteurs de droits externes. La reproduction d'images dans des publications imprimées ou en ligne ainsi que sur des canaux de médias sociaux ou des sites web n'est autorisée qu'avec l'accord préalable des détenteurs des droits. [En savoir plus](#)

### **Terms of use**

The ETH Library is the provider of the digitised journals. It does not own any copyrights to the journals and is not responsible for their content. The rights usually lie with the publishers or the external rights holders. Publishing images in print and online publications, as well as on social media channels or websites, is only permitted with the prior consent of the rights holders. [Find out more](#)

**Download PDF:** 29.03.2026

**ETH-Bibliothek Zürich, E-Periodica, <https://www.e-periodica.ch>**

# Advantages of X-Ray Microanalysis in the Field of Medical Mycology

M. THIBAUT\* and M. ANSEL\*

## *Abstract*

A new apparatus, which combines an electron microprobe and a scanning electron microscope, has been used. This apparatus enabled to conduct a systematic elemental analysis of two species among Aspergillaceae. All elements in the periodic table whose atomic numbers lie between boron and uranium can be detected.

## **Introduction**

Microanalysis by means of X-ray spectrometry allows to detect in a sample all elements of MENDELEEV'S classification comprised between boron and uranium. We deemed it interesting to apply this method to the study of some human pathogenic fungi.

## **Materials and Methods**

### *1 – Basis of the Analytical Method*

The basis of X-ray microanalysis is as follows: the X-ray spectrum emitted under the impact of an electron beam consists on the one hand of a continuous spectrum and on the other hand of a number of characteristic lines that depend on the atoms constituting the anticathode. The small area bombarded in the sample plays the part of the anticathode and sends out, in all directions, X-rays whose spectral analysis is effected by means of spectrometers.

### *2 — Techniques*

The cultures of *Aspergillus clavatus* Desmazieres and *Aspergillus oryzae* (Ah1b) Cohn (both 12 days old) were completely cleared of their food material (Sabouraud infusion). The fragments of mycelium were neither fixed, stained nor embedded. After quick washing in sterile demineralized water, in order to eliminate any traces of nutrient medium, the samples were dried between two sheets of blotting paper and flattened with a weight. The surface of the samples must be as even as possible. The cultures were placed on aluminium cylinders and treated with silver lacquer so as to secure the conductivity of electrons. Then they were placed in a vacuum evaporator where they were coated with a film of aluminium. A coating from 10 nm is generally a desirable range.

For microanalysis, we used the Camebax unit, composed of a modular apparatus for scanning and X-ray microanalysis. This apparatus combines in the same assembly an electron microprobe with three wavelength X-ray spectrometers and a scanning electron microscope. The analysis is performed with the help of an inclined spectrometer that allows to use samples up to 1 mm in diameter.

---

\* Laboratoire de Parasitologie et Mycologie (Pr. M. Larivière), 15, rue de l'Ecole de Médecine, 75006 Paris.

The cultures are analyzed through the combined process of scanning electron microscopy and X-ray spectrometry. After obtaining secondary electron images by means of scanning electron microscopy, some elements belonging to MENDELEEV's periodical classification are investigated by means of wavelength dispersive spectrometry. The X-rays emitted are analyzed with the crystal detectors of spectrometers: pentaerythritol (PET), acid potassium phthalate (KAP) and lithium fluoride (LIF). The conditions required for detection are: accelerating voltage 20 KV, current delivered 50 nA.

## Results

The study of *Aspergillus clavatus* enabled to detect seven elemental chemical components. With the PET crystal detector appeared the specific spectra of the following elements: calcium ( $K\alpha$  line, traces), potassium ( $K\beta$  and  $K\alpha$  lines), chlorine ( $K\alpha$  line), sulphur ( $K\alpha$  line), and phosphorus ( $K\alpha$  line). The Ag  $L\gamma$ ,  $L\beta$  and  $L\alpha$  lines came from the silver lacquer used to stick the samples on the supports. With the KAP crystal detector, the  $K\alpha$  lines of magnesium (traces) and sodium appeared. The Al  $K\alpha$  line came from metallization.

The analysis of *Aspergillus oryzae* showed the presence of eight elements. With the PET crystal detector appeared the specific spectra of calcium ( $K\beta$  and  $K\alpha$  lines), potassium ( $K\alpha$  line), chlorine ( $K\beta$  and  $K\alpha$  lines), sulphur ( $K\alpha$  line) and phosphorus ( $K\alpha$  line). With the KAP crystal detector, silicon ( $K\beta$  and  $K\alpha$  lines), magnesium ( $K\alpha$  line) and sodium ( $K\alpha$  line) were detected. The aluminium  $K\beta$  and  $K\alpha$  lines came from metallization.

In the two species, the LIF crystal detector allowed to detect no element. No other elements of MENDELEEV's periodical classification were detected. But the natural components to be found in living tissues, namely carbon, hydrogen, oxygen and nitrogen, were not investigated. As to the negative results, this technique may not prove useful for infinitesimal quantities.



## Discussion



The history of electron probe microanalysis started with the pioneer work of MOSELEY (1913), who showed that it was possible to detect all elements in the periodic table from their characteristic X-ray emission

---

*Fig. 1.* Analysis of *Aspergillus clavatus* by means of wavelength dispersive spectrometry (Camebax system). With the PET crystal detector are identified: calcium (traces,  $K\alpha$  line), potassium ( $K\beta$  and  $K\alpha$  lines), chlorine, sulphur and phosphorus ( $K\alpha$  lines). The Ag  $L\gamma$ ,  $L\beta$  and  $L\alpha$  lines come from the silver paint used to stick the specimens on the supports.

*Fig. 2.* *Aspergillus clavatus*. Analysis with the KAP crystal detector. The aluminium  $K\alpha$  line comes from metallization. Presence of magnesium (traces) and sodium.

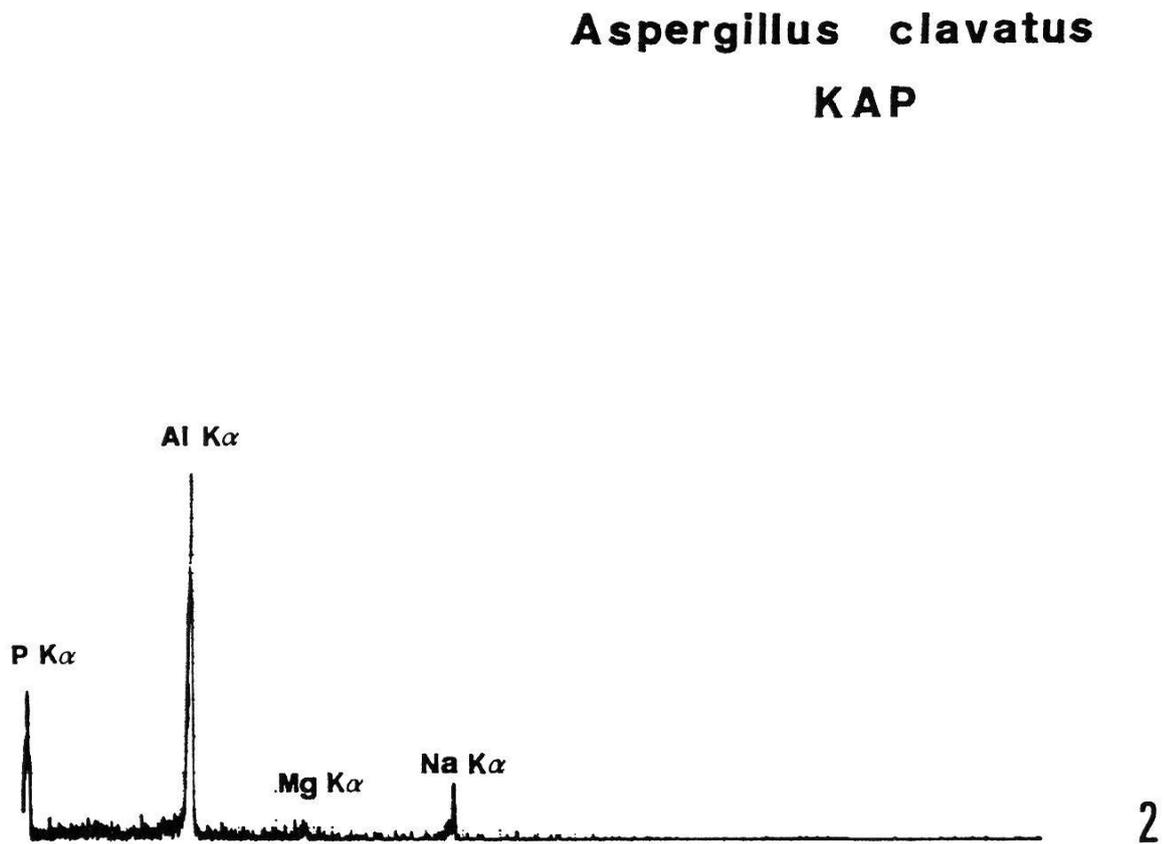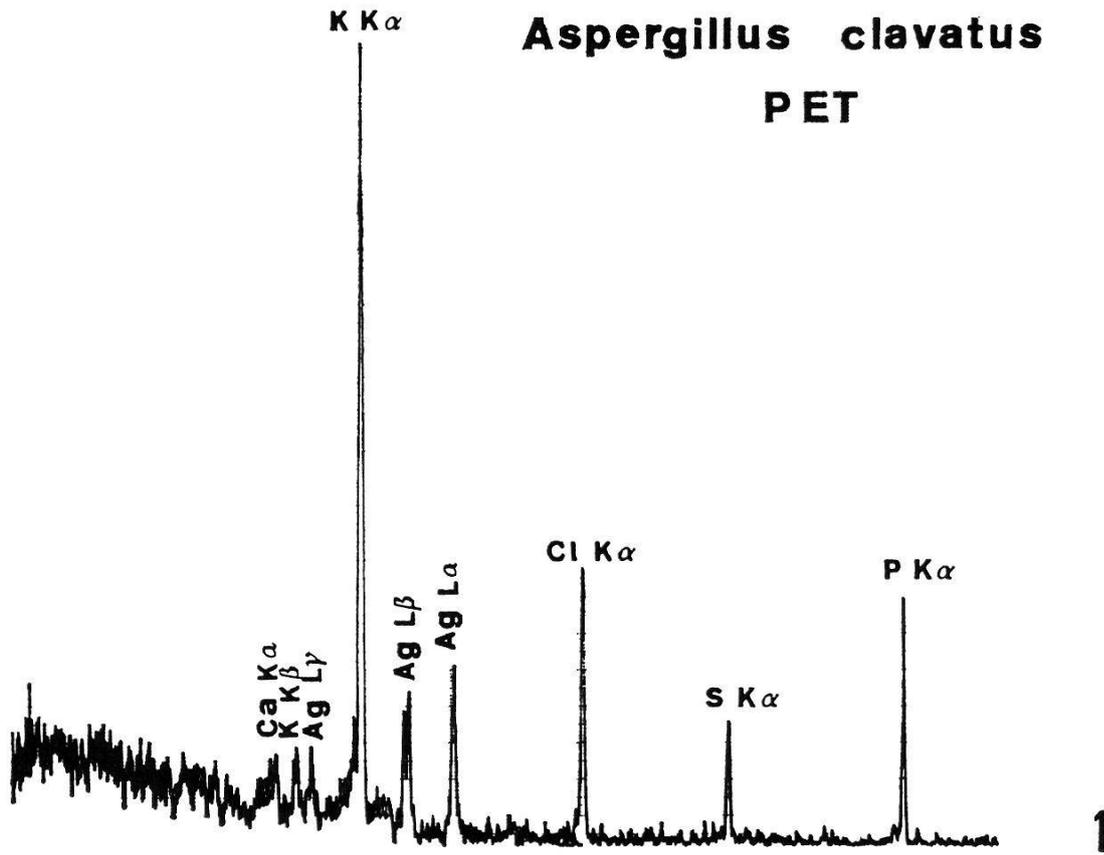

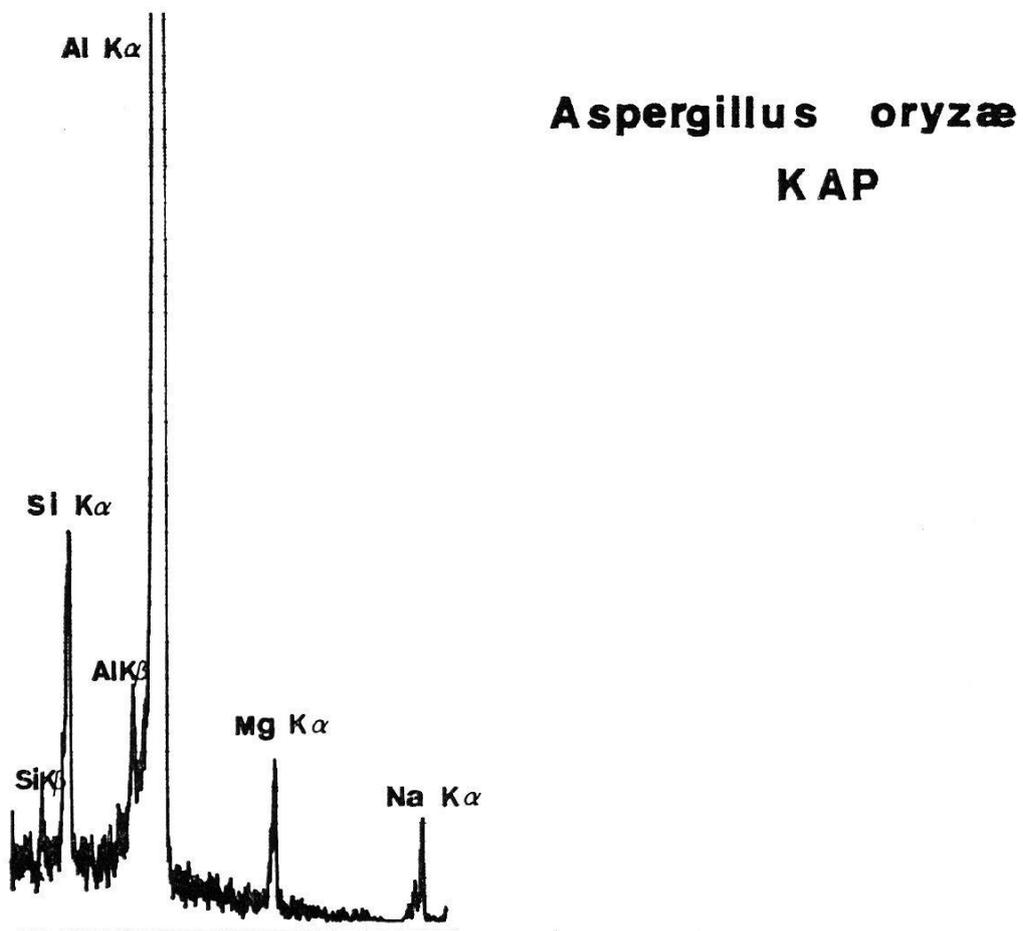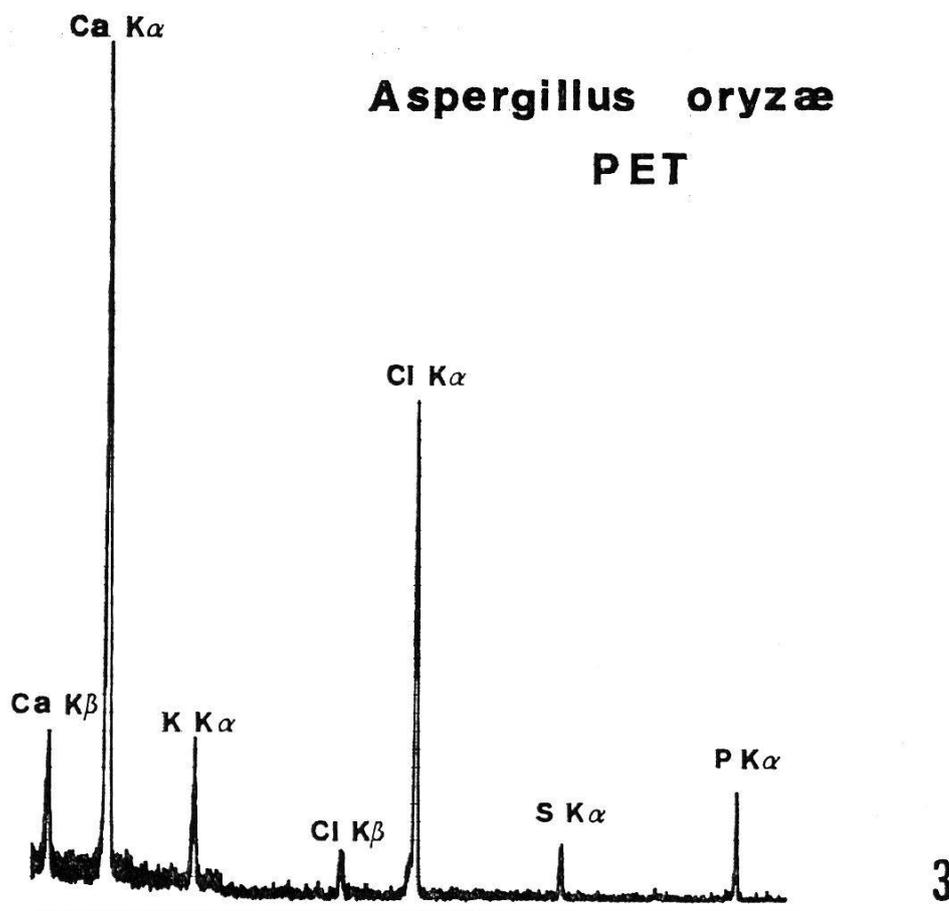

excited by the impact of an electron beam. The application of X-ray spectrometry was developed by CASTAING (1951). In the biological area, it was used notably by GALLE (1965).

In the field of animal biology, X-ray microanalysis was used to detect the distribution of some metals in insects and calcium in the thyroid gland of some mammals (MARTOJA, 1971). Electron microprobe analysis was used to study the cytoplasmic granules in *Tetrahymena pyriformis* (COLEMAN et al., 1972). The refractive bodies in *Amoeba proteus* were studied by means of X-ray spectrometry.

In plant biology, the study of silica in developing epidermal cells of *Avena* internodes was made using electron probe analysis (KAUFMAN et al., 1969). The entry and distribution of aluminium in *Zea mays* was analysed by the same technique (RASMUSSEN, 1969). The localization of aluminium in the cortex cells of bean and barley roots was studied by microanalysis (WAISEL et al., 1970). The structured granules in *Fischerella ambigua* have been investigated by this method (THURSTON & RUSS, 1971). Although X-ray spectrometry has long been used for the elemental analysis of biological specimens, it was not used until recently in medical mycology. The method has been applied to the study of some pathogenic fungi for the detection of their elemental composition (THIBAUT et al., 1974). Thanks to this technique, relevant differences in the natural chemical contents of a number of species of Aspergillaceae were observed (THIBAUT & ANSEL, 1973, 1975).

### Conclusion

Microanalysis by means of X-ray spectrometry enables to obtain chemical information concerning specimens which have not been submitted to fixation, dehydration and embedding and without resorting to a variety of staining methods or different instruments. It makes it possible to study the distribution of periodical elements in biological tissues during the examination of samples by scanning electron microscopy. The analytical electron microscopy enables to observe some differences in the elemental chemical composition of closely related species, for instance *Aspergillus clavatus* and *Aspergillus oryzae*.

---

*Fig. 3. Aspergillus oryzae.* Spectra of calcium ( $K\beta$  and  $K\alpha$  lines), potassium ( $K\alpha$  line), chlorine ( $K\beta$  and  $K\alpha$  lines), sulphur and phosphorus ( $K\alpha$  lines). PET crystal detector.

*Fig. 4. Aspergillus oryzae.* X-ray spectra of silicon ( $K\beta$  and  $K\alpha$  lines), magnesium ( $K\alpha$  line) and sodium ( $K\alpha$  line). The aluminium  $K\beta$  and  $K\alpha$  lines come from metallization. KAP crystal detector.

## Literature cited

- CASTAING, R. (1951). Applications des sondes électroniques à une méthode d'analyse ponctuelle, chimique et cristallographique. – Thèse de Sciences. Paris.
- COLEMAN, J. R., NILSSON, J. R., WARNER, R. R. & BATT, P. (1972). Qualitative and quantitative electron probe analysis of cytoplasmic granules in *Tetrahymena pyriformis*. – Exp. Cell Res. 74, 207.
- COLEMAN, J. R., NILSSON, J. R., WARNER, R. R. & BATT, P. (1973). Electron probe analysis of refractive bodies in *Amoeba proteus*. – Exp. Cell Res. 76, 31.
- GALLE, P. (1965). Analyse chimique ponctuelle des inclusions intra-cellulaires par spectrographie des rayons X. Application à l'étude des cellules rénales. – Thèse de Sciences. Paris. L'Expansion éditeur.
- KAUFMAN, B. P., BIGELOW, W. C., PETERING, L. B. & DROGOS, Z. B. (1969). Silica in developing epidermal cells of *Avena* internodes: Electron probe analysis. – Science 166, 1015.
- MARTOJA, M. (1971). Répartition du calcium dans la glande thyroïde de quelques mammifères. – C. R. Acad. Sci. 272, 3173–3175.
- MARTOJA, R. (1971). Des insectes et des métaux. – La Recherche 18, 1074–1075.
- MOSELEY, H. G. J. (1913). The high frequency spectra of the elements. – Phil. Mag. 26, 1024.
- RASMUSSEN, H. P. (1969). Entry and distribution of aluminium in *Zea mays*. – Planta 81, 28.
- THIBAUT, M. & ANSEL, M. (1973). Mycological applications of X-ray microanalysis. – J. Bact. 116, 1181–1184.
- THIBAUT, M., ANSEL, M. & AZEVEDO DE CARNEIRO, J. DE (1974). Recherches en spectrométrie dispersive sur la composition chimique élémentaire de la phase mycélienne du *Sporothrix schenckii*. – J. Microscopie 20, 93.
- THIBAUT, M. & ANSEL, M. (1975). Constitution chimique élémentaire de deux espèces d'Aspergillaceae étudiées en spectrométrie dispersive. – J. Microscopie Biol. cell. 22, 37.
- THURSTON, E. L. & RUSS, J. C. (1971). Scanning and transmission electron microscopy and microanalysis of structured granules in *Fischerella ambigua*. Scanning electron microscopy. – Proceedings of the fourth annual scanning electron microscope symposium (Chicago, ed. I.I.T. Research Institute).
- WAISEL, Y., HOFFEN, A. & ESHEL, E. (1970). The localization of aluminium in the cortex cells of bean and barley roots by X-ray microanalysis. – Physiol. Plant 23, 75.