

Zeitschrift:	Acta Tropica
Herausgeber:	Schweizerisches Tropeninstitut (Basel)
Band:	45 (1988)
Heft:	1
Artikel:	A new apparatus suitable for the use of counter-immunoelectrophoresis in the field : application for the diagnosis of malaria and leishmaniasis : short communication
Autor:	Monjour, L. / Lecso, G. / Tselentis, Y.
DOI:	https://doi.org/10.5169/seals-314062

Nutzungsbedingungen

Die ETH-Bibliothek ist die Anbieterin der digitalisierten Zeitschriften auf E-Periodica. Sie besitzt keine Urheberrechte an den Zeitschriften und ist nicht verantwortlich für deren Inhalte. Die Rechte liegen in der Regel bei den Herausgebern beziehungsweise den externen Rechteinhabern. Das Veröffentlichen von Bildern in Print- und Online-Publikationen sowie auf Social Media-Kanälen oder Webseiten ist nur mit vorheriger Genehmigung der Rechteinhaber erlaubt. [Mehr erfahren](#)

Conditions d'utilisation

L'ETH Library est le fournisseur des revues numérisées. Elle ne détient aucun droit d'auteur sur les revues et n'est pas responsable de leur contenu. En règle générale, les droits sont détenus par les éditeurs ou les détenteurs de droits externes. La reproduction d'images dans des publications imprimées ou en ligne ainsi que sur des canaux de médias sociaux ou des sites web n'est autorisée qu'avec l'accord préalable des détenteurs des droits. [En savoir plus](#)

Terms of use

The ETH Library is the provider of the digitised journals. It does not own any copyrights to the journals and is not responsible for their content. The rights usually lie with the publishers or the external rights holders. Publishing images in print and online publications, as well as on social media channels or websites, is only permitted with the prior consent of the rights holders. [Find out more](#)

Download PDF: 06.08.2025

ETH-Bibliothek Zürich, E-Periodica, <https://www.e-periodica.ch>

¹ Laboratoire de Parasitologie expérimentale et INSERM U 313,

Faculté de Médecine Pitié-Salpêtrière, Paris, France

² Laboratoire de Parasitologie, Hôpital Laïkon, Gaudi – Athènes, Grèce

A new apparatus suitable for the use of counter-immunoelectrophoresis in the field: application for the diagnosis of malaria and leishmaniasis

Short communication

L. MONJOUR¹, G. LECSO¹, Y. TSELENTIS², D. MAZIER¹, I. VOULDOUKIS¹,
C. ALFRED¹, C. DANIEL-RIBEIRO¹, D. FROMMEL¹

Counterimmunoelectrophoresis (CIE) has been applied for establishing the diagnosis of infectious diseases. Its application was first undertaken with agar or agarose gels as support for the electrophoretic run (see Guinet, 1978). In the authors' laboratory, CIE was modified by using, instead of agarose gels, cellulose acetate membranes (Gentilini et al., 1972). Routinely employed for the detection of parasitic (Druilhe et al., 1978; Monjour et al., 1978) and fungal (Monjour et al., 1975, 1978) antibodies in patient sera, we demonstrate that CIE can be easily adapted to malaria and leishmaniasis surveys conducted in rural areas, in the field.

The first survey was conducted in Burkina Faso, near Ouagadougou. 629 sera of countrymen living in a malaria holoendemic area were tested for malaria antibodies. The second survey was carried out in Greece, around Athens. 260 sera (humans = 200; dogs = 60) were collected for the detection of Leishmania antibodies. All sera were immediately studied in the field by CIE and later, in our laboratory, by CIE and indirect immunofluorescence (IFI).

Leishmania infantum promastigotes were cultured and used as antigens for CIE and IFI as previously described (Monjour et al., 1978). For malaria survey, these two techniques (Druilhe et al., 1978) were employed with parasitized red blood cells (PRBC) from a *Plasmodium falciparum* malaria patient. In our laboratory previous studies based on 150 cases of visceral leishmaniasis, 3000 sera of malaria patients and 7000 sera of subjects with parasitic and non-parasitic infections, showed that CIE has a specificity and a sensitivity equivalent, if not higher, than IFI (unpublished results). Moreover, the rapidity of the CIE method (around 3 h for a serological diagnosis) can easily allow collective detection in village populations.

The usual CIE technique requires standard equipment, comprising electrophoretic tanks (Chemetron – tank mod. 2, pac 5), cellulose acetate membranes (Sebia strips 17 cm × 2,5 cm × 200 µ), the antigens and test sera (Gentilini et al., 1972). For application in the field, in areas devoid of any electricity supply, we adopted the following set-up: a standard 12 volts car battery (45 Amps/h), a fitting for an 8 W fluorescent tube (12 volts D.C. – Mazda & Co.; ref. RBIC 8 T 12), a bridge rectifier (1 Amp., 1000 Volts), an electrolytic capacitor: 200 µF; 180 volts; a potentiometer 10 K Ω; 5 W (Fig. 1). The fitting was used as a current converter to increase the voltage from 12 to around 100 volts in order to obtain rapid electrophoretic migrations. The potentiometer enabled the voltage to be

Correspondence: Dr Loïc Monjour, Laboratoire de Parasitologie expérimentale et INSERM U 313, Faculté de Médecine Pitié-Salpêtrière, 47, Bd de l'Hôpital, F-75834 Paris Cedex 13, France

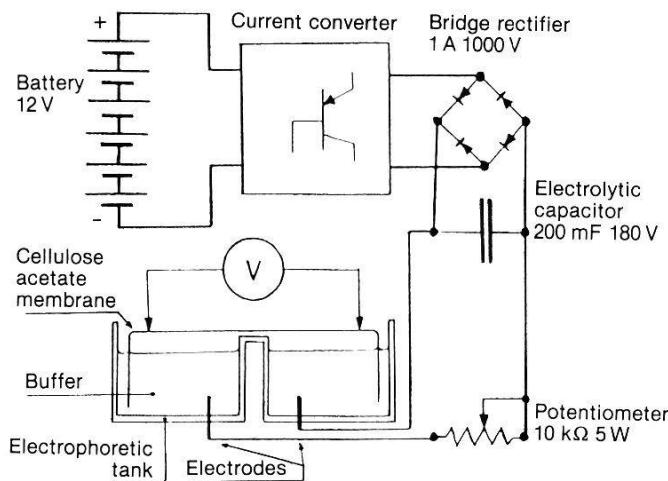


Fig. 1. Ad hoc equipment for the counterimmuno-electrophoresis technique performed in the field.

adjusted as required, between 60 and 75 volts measured at both ends of the cellulose acetate strips. All the equipment involved was encased in a metal envelope for protection.

Results of the CIE technique applied in the field were confirmed in the laboratory with a conventional set-up. In Greece, one already known leishmanian patient (CIE +; IFI reciprocal titer [IRT] = 800) and 3 dogs (CIE +; IRT = 800, 800 and 1600) were proven to be serologically positive. The canine leishmanias were confirmed by the presence of amastigotes in bone-marrow aspirates. In Burkina Faso, malaria antibodies were demonstrated by the two techniques for 625 subjects. Four sera were subject to discussion = 2 CIE negative and IFI weakly positive and vice-versa for the two others. In this study, the IFI positive titer range extended from 800 to 25,600.

The value of CIE, has been considered in terms of output. The test was perfectly feasible for up to 400 sera without exploiting the total electricity supply of the battery; it is time-saving, allowing diagnosis of the disease and beginning of the treatment on the same day; lastly, the cost per examination amounts to no more than 0.30 US dollar.

Acknowledgments. This work was supported by a grant from the Ministère des Relations Extérieures (Sous-Direction de la Recherche et de l'Information Scientifiques – France).

Druilhe P., Monjour L., Richard-Lenoble D., Gentilini M.: L'immuno-électro-diffusion sur membrane d'acétate de cellulose pour le diagnostic sérologique du paludisme humain. Path. Biol. 26, 169–172 (1978).

Gentilini M., Pinon J. M., Niel G.: Immuno-électro-diffusion sur membrane d'acétate de cellulose. Application en parasitologie. Bull. Soc. Path. exot. 63, 60–66 (1972).

Guinet R.: L'électrosynthèse et ses applications. Rev. Inst. Pasteur (Lyon) 11, 1–33 (1978).

Monjour L., Niel G., Dautry J., Briand A., Gentilini M.: Application de l'électrosynthèse, sur membrane d'acétate de cellulose, au diagnostic des aspergilloses. Bull. Soc. Myc. méd. 4, 225–230 (1975).

Monjour L., Mille C., Druilhe P., Gentilini M.: Application de l'immuno-électro-diffusion sur membrane d'acétate de cellulose au diagnostic de la leishmaniose viscérale humaine et canine. Ann. Soc. belge Méd. trop. 58, 293–300 (1978).

Monjour L., Mogahed A., Druilhe P., Gentilini M.: Application de l'immuno-électro-diffusion sur membrane d'acétate de cellulose, au diagnostic des candidoses. Valeur des antigènes standardisés et résultats comparatifs avec l'immunodiffusion et l'hémagglutination passive. Bull. Soc. Myc. méd. 1, 45–52 (1978).

Monjour L., Mille C., Druilhe P., Gentilini M.: Préparation, à partir d'un milieu de culture modifié, des antigènes somatique et métabolique de *Leishmania donovani*. Ann. Soc. belge Méd. trop. 58, 287–290 (1978).